

CLINICS-D-25-01163

Supplemental Material

Table S1 Results of Egger's test for all outcomes.

Outcomes	p for Egger's test	Publication bias
Short time mortality	0.781	No
Proportion of RRT	0.477	No
24-hour lactate level	0.744	No
24-hour lactate change	0.538	No
24-hour SOFA score change	0.367	No

Figure S1 Sensitivity analysis for short time mortality.

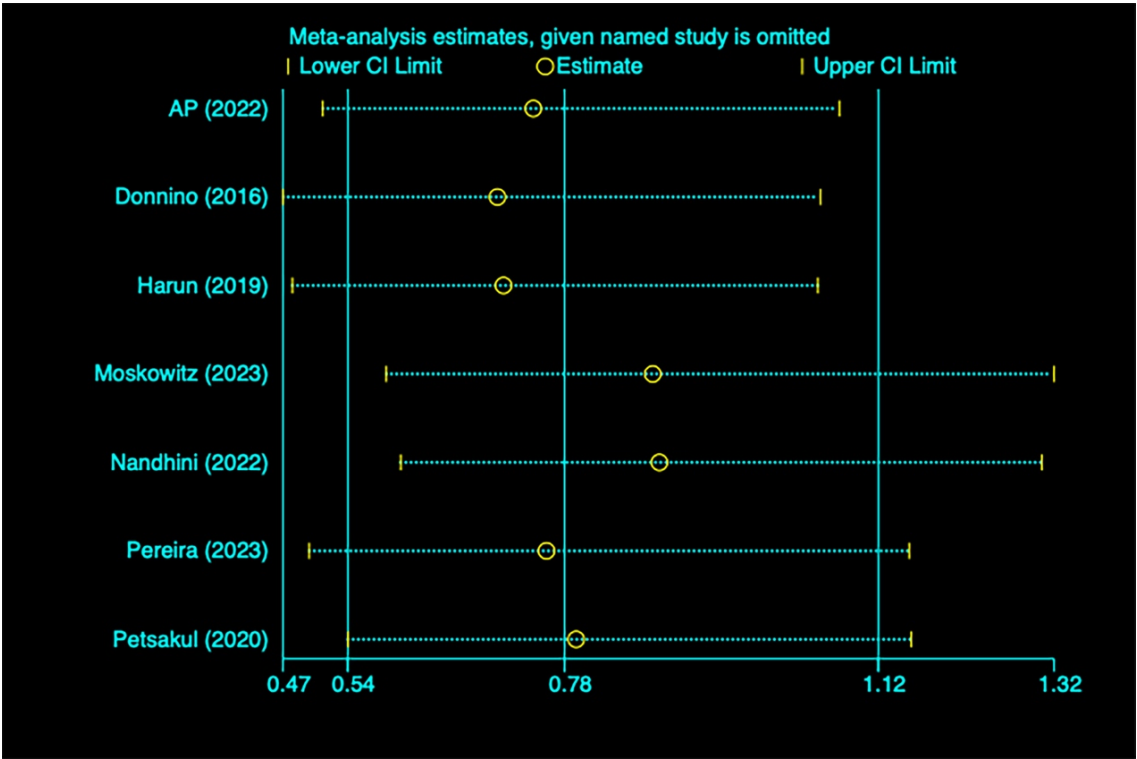


Figure S2 Sensitivity analysis for the proportion of renal replacement therapy.

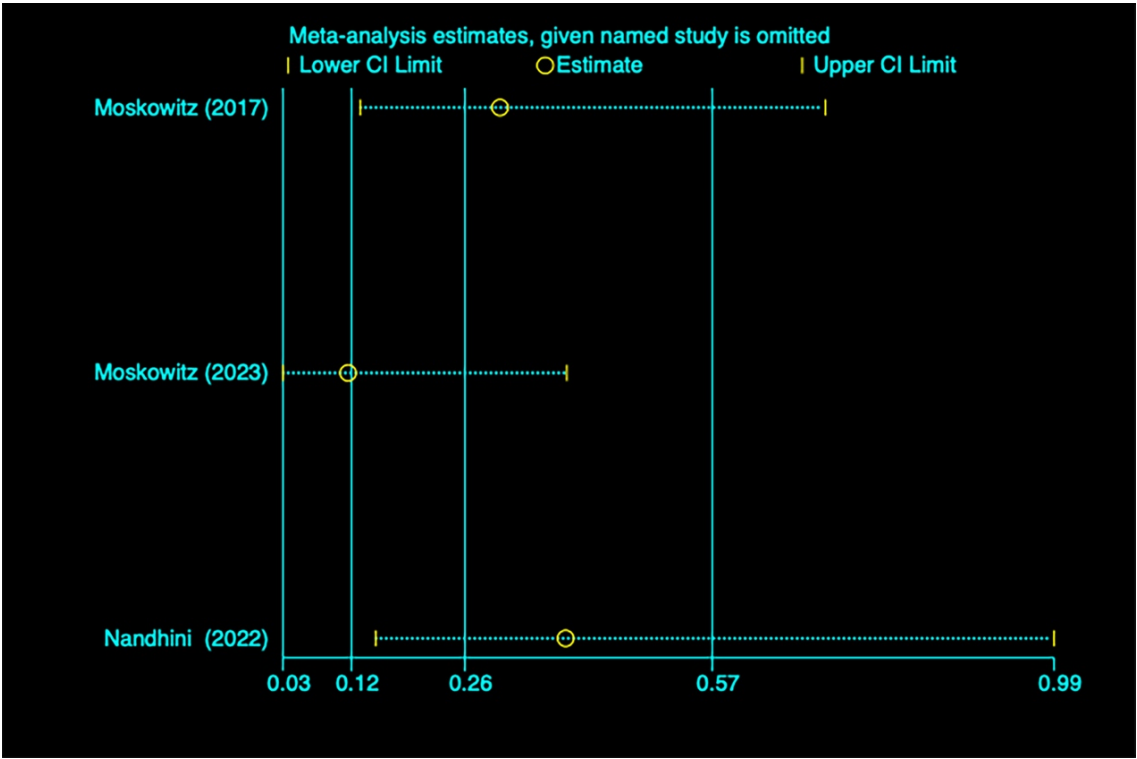


Figure S3 Sensitivity analysis for the 24-hour lactate level.

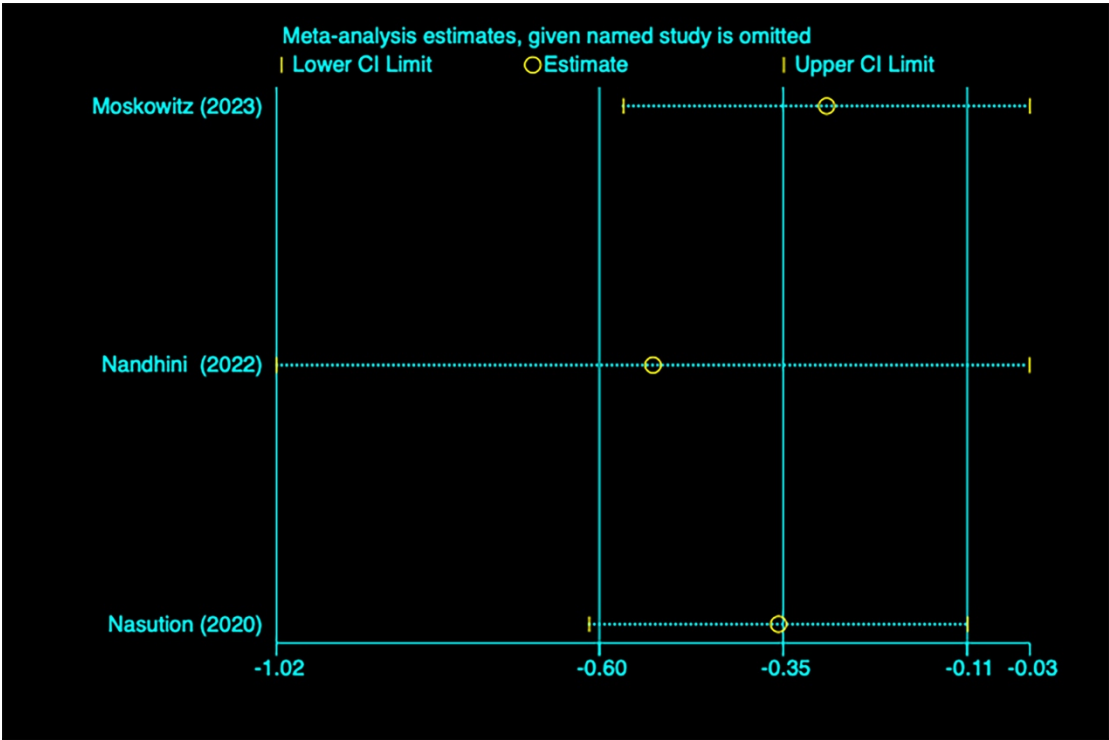


Figure S4 Sensitivity analysis for the 24-hour lactate change.

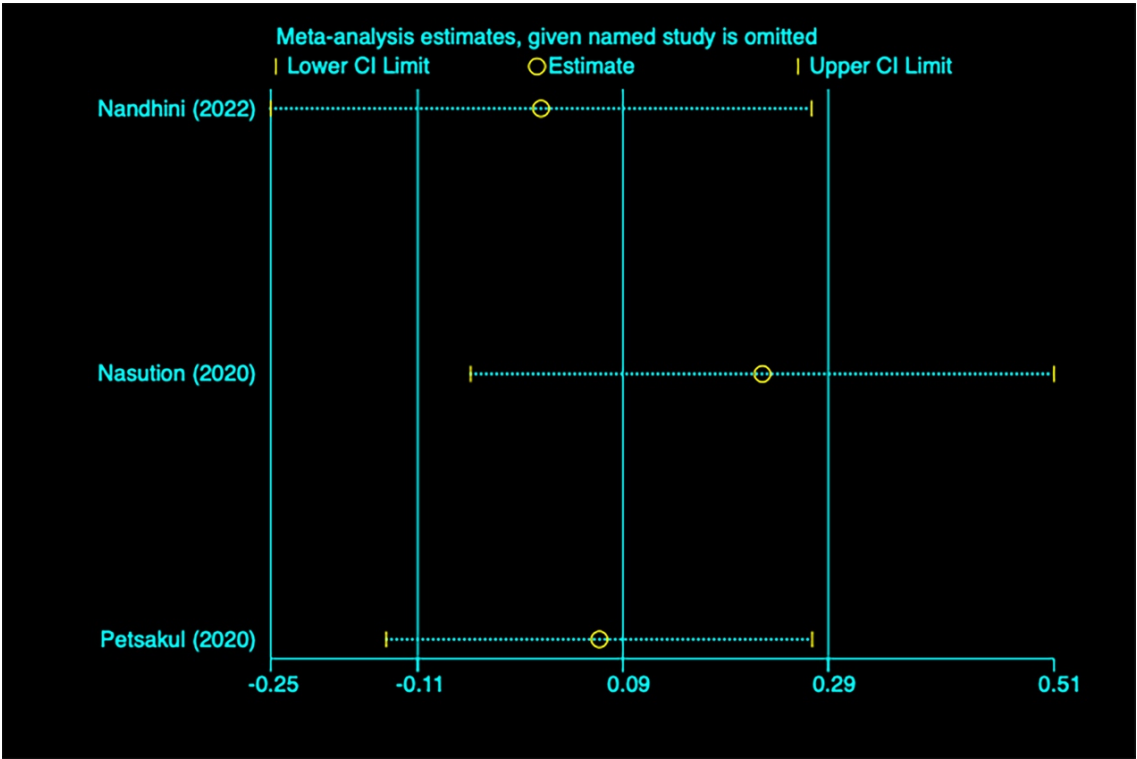


Figure S5 Sensitivity analysis for the 24-hour sequential organ failure assessment change.

